

**LOGOSCREEN** es

Paperless Recorder  
for secure acquisition of  
FDA-compliant  
measurement data

B 70.6560.2.3  
PROFIBUS DP  
Interface Description



<b>1</b>	<b>Introduction</b>	<b>5</b>
1.1	Preface .....	5
1.2	Typographical conventions .....	6
1.2.1	Warnings .....	6
1.2.2	Note signs .....	6
<b>2</b>	<b>Profibus description</b>	<b>7</b>
2.1	Profibus types .....	7
2.2	RS485 transmission technology .....	8
2.3	PROFIBUS DP .....	11
<b>3</b>	<b>Configuring a PROFIBUS system</b>	<b>13</b>
3.1	GSD files .....	13
3.2	Configuration procedure .....	14
3.3	The GSD generator .....	15
3.3.1	General .....	15
3.3.2	Operation .....	15
3.3.3	Example report .....	17
3.4	Connection example .....	19
3.4.1	RECORDER .....	19
3.4.2	GSD generator .....	19
3.4.3	PLC configuration .....	20
<b>4</b>	<b>Data format of the recorder</b>	<b>23</b>
<b>5</b>	<b>Device-specific data</b>	<b>25</b>
5.1	Paperless recorder LOGOSCREEN .....	26
5.2	System requirements .....	26
5.3	Connection diagram .....	26
5.4	Setting the slave address .....	27
5.5	Diagnostic and status messages .....	27
5.6	Acyclic data .....	27
5.7	PLC data in 16-bit format .....	32

---

# Contents

---

<b>5.8</b>	<b>Bit-by-bit coding of binary signals .....</b>	<b>34</b>
<b>5.9</b>	<b>External inputs and faults in the data exchange .....</b>	<b>35</b>
<b>5.10</b>	<b>Paperless recorders LOGOSCREEN es and cf .....</b>	<b>36</b>
5.10.1	System requirements .....	36
5.10.2	Connections for LOGOSCREEN es and cf .....	36
5.10.3	Setting the slave address .....	37
5.10.4	Diagnosis and status messages .....	37
5.10.5	Acyclic data transmission .....	37
5.10.6	Extension of the address range for LOGOSCREEN es and cf .....	38
5.10.7	Process data .....	39
5.10.8	PLC data in 16-bit format .....	46
5.10.9	Bit-wise coded binary logic signals .....	48
5.10.10	External inputs and faults in the data exchange .....	49

## 1.1 Preface



Please read this manual before starting up the interface. Keep the manual in a place which is accessible to all users at all times.

Please assist us to improve this manual.

Your suggestions will be welcome.



If any difficulties should arise during commissioning, you are asked not to carry out any unauthorized manipulations. You could endanger your rights under the instrument warranty!

Please contact the nearest subsidiary or the main factory in such a case.



When returning chassis, modules or components, the regulations of EN 100 015 "Protection of electrostatically sensitive components" must be observed. Use only the appropriate **ESD** packaging for transport.

Please note that we cannot accept any liability for damage caused by ESD (electrostatic discharge).

# 1 Introduction

---

## 1.2 Typographical conventions

### 1.2.1 Warnings

The signs for **Danger** and **Caution** are used in this manual under the following conditions:



#### **Danger**

This symbol is used where there may be **danger to personnel** if the instructions are disregarded or not followed accurately!



#### **Caution**

This symbol is used where there may be **damage to equipment or data** if the instructions are disregarded or not followed accurately!



#### **Caution**

This symbol is used if precautions must be taken when handling **electrostatically sensitive components**.

### 1.2.2 Note signs



#### **Note**

This symbol is used to draw your **special attention** to a remark.



#### **Reference**

This symbol refers to **additional information** in other manuals, chapters or sections.

abc<sup>1</sup>

#### **Footnote**

Footnotes are notes which **refer to certain points** in the text. Footnotes consist of two parts:


Marking in the text and the footnote text.

The marking in the text is arranged as continuous superscript numbers.

#### **Handling instructions**

This symbol marks the description of a **required action**.

The individual steps are indicated by an asterisk, e. g.

\* Press the  key

\* Confirm with 


\*

## 2 Profibus description

PROFIBUS is a manufacturer-independent, open fieldbus standard for a wide range of applications in manufacturing, process and building automation. Manufacturer independence and openness are ensured by the international standard EN 50 170.

Using PROFIBUS, devices from different manufacturers can communicate without any special interface adjustments. PROFIBUS can be employed for both high-speed time-critical data transmission and extensive, complex communication tasks. The PROFIBUS family consists of three versions.

### 2.1 Profibus types

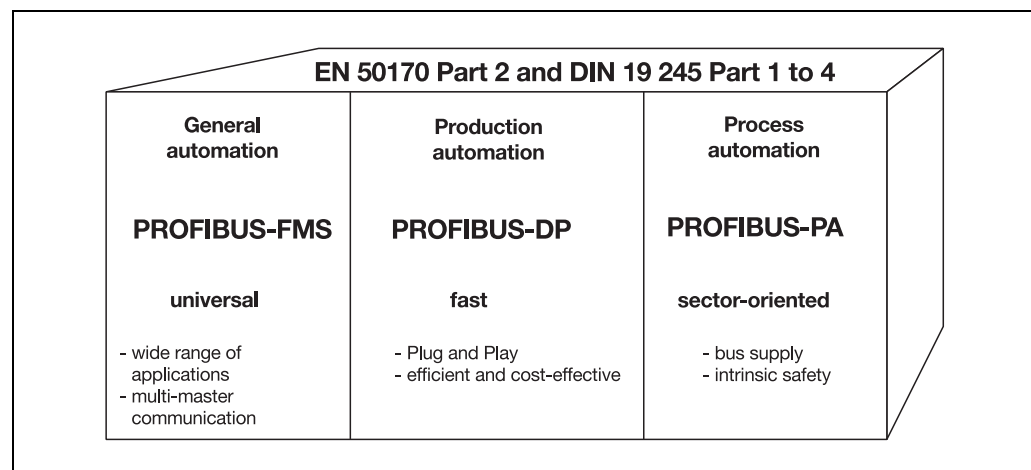

**The PROFIBUS family**

#### **PROFIBUS DP**

This PROFIBUS version, which is optimized for high speed and low connection costs, has been especially designed for communication between automation control systems (PLC) and distributed field devices (typical access time: < 10msec). PROFIBUS DP can be used to replace conventional, parallel signal transmission with 24V or 0/4–20mA.

DPV0: cyclic data transfer:  
--> is supported by the recorder.

DPV1: cyclic and acyclic data transfer:  
--> is not supported by the recorder.

DPV2: slave-to-slave communication takes place in addition to cyclic and acyclic data transfer:  
--> is not supported by the recorder.

#### **PROFIBUS-PA**

PROFIBUS-PA has been specifically designed for process engineering. It permits the linking of sensors and actuators to a common bus cable, even in hazardous areas. PROFIBUS-PA enables the data communication and energy supply for devices in two-wire technology according to the international IEC 1158-2 standard.

#### **PROFIBUS-FMS**

This is the universal solution for communication tasks at cell level (typical access time: approx. 100msec). The powerful FMS services open up a wide range of applications and provide a high degree of flexibility. FMS is also suitable for extensive communication tasks.

## 2 Profibus description

---

### 2.2 RS485 transmission technology

Transmission takes place according to the RS485 standard. It covers all areas in which a high transmission speed and simple, cost-effective installation are required. A shielded twisted copper cable with one conductor pair is used.

The bus structure permits addition and removal of stations or step-by-step commissioning of the system without affecting the other stations. Later expansions have no influence on the stations which are already in operation.

Transmission speeds between 9.6 kbit/sec and 12 Mbit/sec are available. One uniform transmission speed is selected for all devices on the bus when the system is commissioned.

Network topology	linear bus, active bus termination at both ends, stub cables are only permissible for baud rates $\leq 1.5$ Mbit/sec.
Medium	shielded twisted-pair cable
Number of stations	32 stations in each segment without repeater (line amplifier). With repeaters, this can be expanded to 126.
Connector	preferably 9-pin sub-D connector

#### Basic features of the RS485 transmission technology

#### Installation tips

All devices are connected in a bus structure (line). Up to 32 stations (master or slaves) can be linked up in one segment.

The bus is terminated by an active bus terminator at the start and end of each segment. Both bus terminators must always be powered, to ensure fault-free operation.

If there are more than 32 users, repeaters must be used to link up the individual bus segments.

## 2 Profibus description

---

**Cable length** The maximum cable length depends on the transmission speed. The cable length specified can be extended by using repeaters. It is recommended not to connect more than 3 repeaters in series.

Baud rate (kbit/s)	9.6	19.2	93.75	187.5	500	1500	12000
Range/segment	1200 m	1200 m	1200 m	1000 m	400 m	200 m	100 m

### Range based on transmission speed

**Cable data** These cable length specifications refer to the cable type described below:

Characteristic impedance:	135 — 165 $\Omega$
Capacitance per unit length:	< 30 pf/m
Loop resistance:	110 $\Omega$ /km
Core dia.:	0.64 mm
Core cross-section:	> 0.34 mm <sup>2</sup>

It is preferable to use a 9-pin sub-D connector for PROFIBUS networks incorporating RS485 transmission technology. The pin assignment at the connector and the wiring are shown at the end of this chapter.

PROFIBUS cables and connectors are supplied by several manufacturers. Please refer to the PROFIBUS product catalog ([www.profibus.com](http://www.profibus.com)) for types and addresses of suppliers.

When connecting up the devices, make sure that the data lines are not reversed. It is absolutely essential to use shielded data lines. The braided shield and the screen foil underneath (if present) should be connected to the protective earth on both sides, and with good conductivity. Furthermore, the data lines should be routed separately from all high-voltage cables, as far as this is possible.

As a suitable cable we recommend the following type from Siemens:

**Simatic Net Profibus 6XV1**

**Order No. 830-0AH10**

**\* (UL) CMX 75 °C (Shielded) AWG 22 \***

## 2 Profibus description

### Data rate

For installation, the use of stub cables must be avoided for data rates above 1.5 Mbit/sec.



For important tips on installation, please refer to the Installation Guidelines PROFIBUS DP, Order No. 2.111 by the PNO (Profibus User Organization).


Address:  
Profibus Nutzerorganisation e.V.  
Haid- u. Neu-Straße 7  
D-76131 Karlsruhe, Germany

Internet: [www.profibus.com](http://www.profibus.com)

### Recommendation:

**Please follow the installation recommendations made by the PNO, especially for the simultaneous use of frequency inverters.**

### Wiring and bus termination

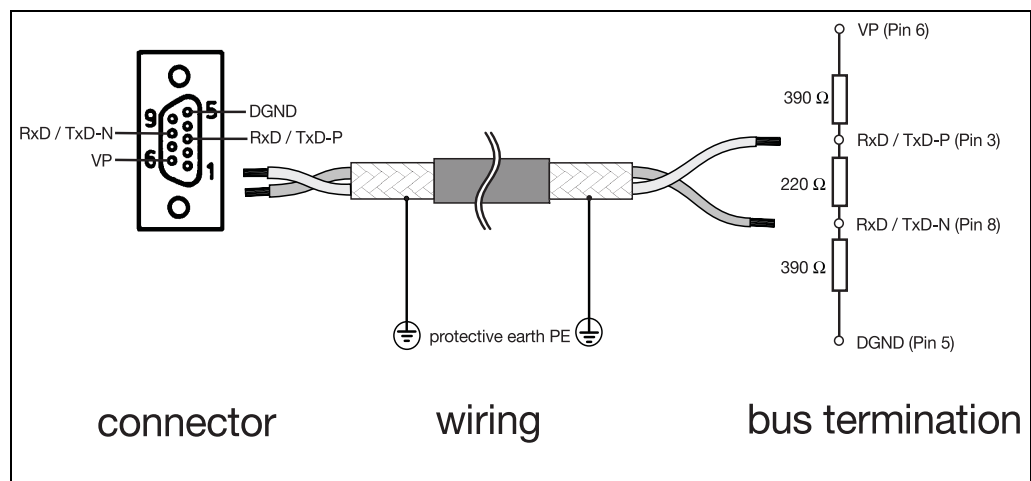

### 2.3 PROFIBUS DP

PROFIBUS DP is designed for high-speed data exchange at the field level. The central control devices, PLC/PC for instance, communicate through a fast serial connection with distributed field devices such as I/O, paperless recorders and controllers. Data exchange with these distributed devices is mainly cyclic. The communication functions required for this are defined by the basic PROFIBUS DP functions in accordance with EN 50 170.

#### Basic functions

The central controller (master) reads the input information cyclically from the slaves and writes the output information cyclically to the slaves. The bus cycle time must be shorter than the program cycle time of the central PLC. In addition to cyclic user data transmission, PROFIBUS DP provides powerful functions for diagnostics and commissioning.


<b>Transmission technology:</b> <ul style="list-style-type: none"><li>• RS485 twisted pair</li><li>• Baud rates from 9.6 kbit/sec up to 12 Mbit/sec</li></ul>
<b>Bus access:</b> <ul style="list-style-type: none"><li>• Master and slave devices, max. 126 users on one bus</li></ul>
<b>Communication:</b> <ul style="list-style-type: none"><li>• Peer-to-peer (user data communication)</li><li>• Cyclic master-slave user data communication</li></ul>
<b>Operating states:</b> <ul style="list-style-type: none"><li>• Operate: Cyclic transmission of input and output data</li><li>• Clear: Inputs are read, outputs remain in secure state</li><li>• Stop: Only master-master data transfer is possible</li></ul>
<b>Synchronization:</b> <ul style="list-style-type: none"><li>• Sync mode: not supported by the recorder</li><li>• Freeze mode: not supported by the recorder</li></ul>
<b>Functionality:</b> <ul style="list-style-type: none"><li>• Cyclic user data transfer between DP master and DP slave(s)</li><li>• Dynamic activation or deactivation of individual DP slaves</li><li>• Checking the configuration of the DP slaves</li><li>• Address assignment for the DP slaves via the bus</li><li>• Configuration of the DP master via the bus</li><li>• maximum of 246 bytes input/output data for each DP slave</li></ul>
<b>Protective functions:</b> <ul style="list-style-type: none"><li>• Address monitoring for the DP slaves</li><li>• Access protection for inputs/outputs of the DP slaves</li><li>• Monitoring of user data communication with adjustable monitoring timer in the master</li></ul>
<b>Device types:</b> <ul style="list-style-type: none"><li>• DP master Class 2, e. g. programming/project design devices</li><li>• DP master Class 1, e. g. central automation devices such as PLC, PC...</li><li>• DP slave e. g. devices with binary or analog inputs/outputs, controllers, recorders...</li></ul>

## 2 Profibus description

### Cyclic data transmission

The data transmission between the master and the DP slaves is carried out by the master in a defined, recurring order. When configuring the bus system, the user defines the assignment of a DP slave to the master. It is also defined which DP slaves are to be included in, or excluded from, the cyclic user data communication.

Data transmission between the master and the DP slaves is divided into three phases: parameterization, configuration and data transfer. Before a DP slave enters the data transfer phase, the master checks in the parameterization and configuration phase whether the planned configuration matches the actual device configuration. In the course of this check, the device type, format and length information, as well as the number of inputs and outputs must agree. These checks provide the user with reliable protection against parameterization errors. In addition to the user data transfer, which is performed automatically by the master, new parameterization data can be sent to the DP slaves at the request of the user.

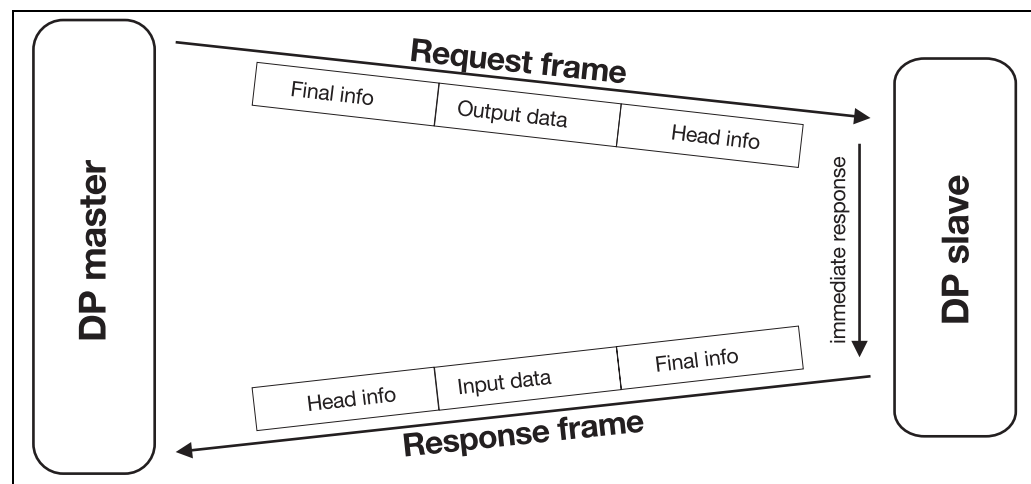

User data transmission in PROFIBUS DP

# 3 Configuring a PROFIBUS system

---

## 3.1 GSD files

Device base data (GSD) enable open project design.

PROFIBUS devices have different features. They differ with respect to the available functionality (e. g. number of I/O signals, diagnostic messages) or possible bus parameters, such as baud rate and time monitoring. These parameters vary individually for each device type and manufacturer. In order to obtain simple Plug & Play configuration for PROFIBUS, the characteristic device features are defined in an electronic device data sheet (Device Data Base File, GSD file). The standardized GSD files expand open communication up to the operator level. By means of the project design tool, which is based on the GSD files, devices from different manufacturers can be integrated into a bus system, simply and user-friendly. The GSD files provide a clear and comprehensive description of a device type in a precisely defined format. GSD files are prepared according to the application. The defined data format permits the project design system to simply read in the GSD files of any PROFIBUS DP device and automatically use this information when configuring the bus system. Already during the project design phase, the project design system can automatically perform checks for input errors and the consistency of data entered in relation to the entire system.

The GSD files are divided into three sections.

- **General specifications**  
This section contains information on manufacturer and device names, hardware and software release states, baud rates supported and the possible time intervals for monitoring times.
- **DP master-related specifications**  
This section contains all the parameters related to DP-master devices only, such as the maximum number of DP slaves that can be connected, or upload and download options. This section is not available for slave devices.
- **DP-slave related specifications**  
This section contains all slave-related specifications, such as the number and type of the I/O channels, specification of diagnostic texts and information on the consistency of I/O data.

The GSD format is designed for flexibility. It contains lists, such as the baud rates supported by the device, as well as the possibility of describing the modules available in a modular device.

# 3 Configuring a PROFIBUS system


## 3.2 Configuration procedure

### Plug & Play

To simplify the configuration of the PROFIBUS system, the master (PLC) is configured using the PROFIBUS configurator and the GSD files, or in the PLC through the hardware configurator.

#### Configuration steps:

- Create GSD file by using the GSD generator
- Load GSD files of the PROFIBUS slaves into the PROFIBUS network configuration software
- Perform configuration
- Load configuration into the system (e.g. PLC)

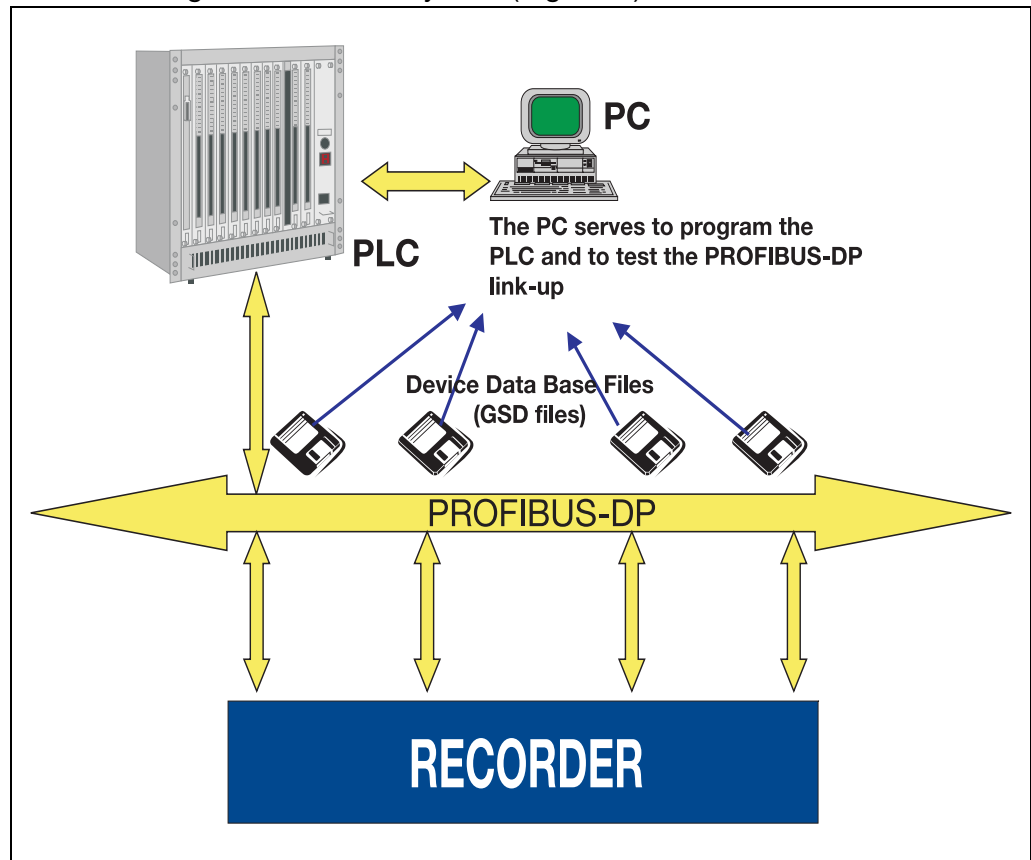

### The GSD file

The characteristic device features of a PROFIBUS slave are specified by the manufacturer, clearly and comprehensively in a precisely defined format, in the GSD file (Device Data Base File).

### The PROFIBUS configurator / hardware configurator (PLC)

This software can read in the GSD files for PROFIBUS DP devices of any manufacturer and integrate them for the configuration of the bus system.

Already in the project design phase, the PROFIBUS configurator automatically checks the files that have been entered for errors in system consistency.

The result of the configuration is read into the master (PLC).

# 3 Configuring a PROFIBUS system

## 3.3 The GSD generator


### 3.3.1 General

GSD files for recorders with a PROFIBUS interface are generated by the user with the aid of the GSD generator.

The recorders with a PROFIBUS interface can send or receive a large variety of variables (parameters). Since, however, in most applications, only a portion of these variables will be sent via PROFIBUS, the GSD generator makes a selection of these variables.

After selection of the device, all available variables are shown in the “Parameters” window. Only after these have been copied to the “Input” or “Output” window will they later be contained in the GSD file for processing or pre-processing by the master (PLC).


### 3.3.2 Operation

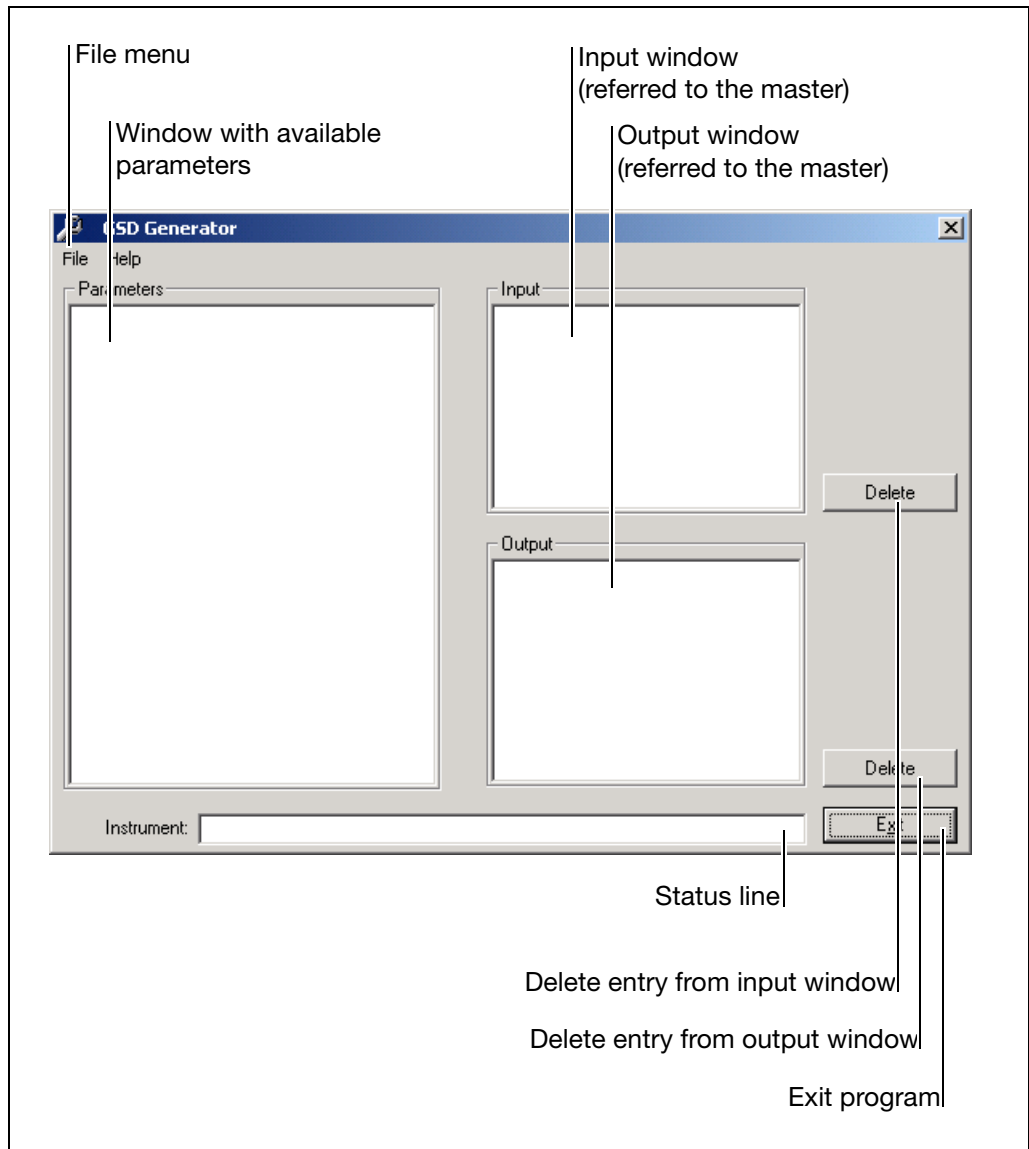

### 3 Configuring a PROFIBUS system

**File menu**

The file menu can be called up using the Alt-D combination or the left mouse button. It provides the following options:

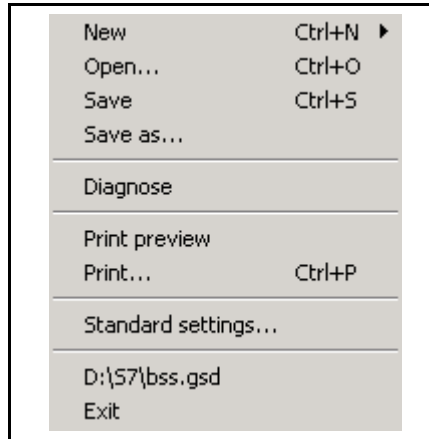

<b>New</b>	After calling up the function which creates a new GSD file, the available devices are selected. After selection of the required device, all available parameters are shown in the parameter window.
<b>Open</b>	This function opens an existing GSD file.
<b>Save/ Save as</b>	This function is available for saving the generated or altered GSD file.
<b>Diagnosis</b>	Using this function, the GSD file can be tested in conjunction with a PROFIBUS DP adapter from B+W.
<b>Print preview</b>	shows the preview of a report <sup>1</sup> that can be printed.
<b>Print</b>	prints a report <sup>1</sup> .
<b>Standard settings</b>	The language to be used at the next restart of the program can be selected here.
<b>Exit</b>	exits the program.



<sup>1</sup>. The report contains additional information for the PLC programmer (e.g. data type of the selected parameters).

⇒ Chapter 3.3.3 “Example report”

## 3 Configuring a PROFIBUS system

---

### 3.3.3 Example report

I/O report

Device: RECORDER

Length of inputs (byte): 7

Length of outputs (byte): 4

Inputs

Byte	Description	Type
-----		
[ 0]	Interface status	BYTE
[ 1]	int. logic inputs\Bool_Out01	BOOLEAN
[ 2]	int. logic inputs\Bool_Out02	BOOLEAN
[ 3]	int. analog inputs 16Bit\Int_Out01	INTEGER
[ 5]	int. analog inputs 16Bit\Int_Out02	INTEGER


Outputs

Byte	Description	Type
-----		
[ 0]	ext. analog inputs 16Bit\Int_In01	INTEGER
[ 2]	ext. analog inputs 16Bit\Int_In02	INTEGER

# 3 Configuring a PROFIBUS system

## Select parameter

If an existing file has been opened, or a new one created, all available parameters are shown in the parameter window.

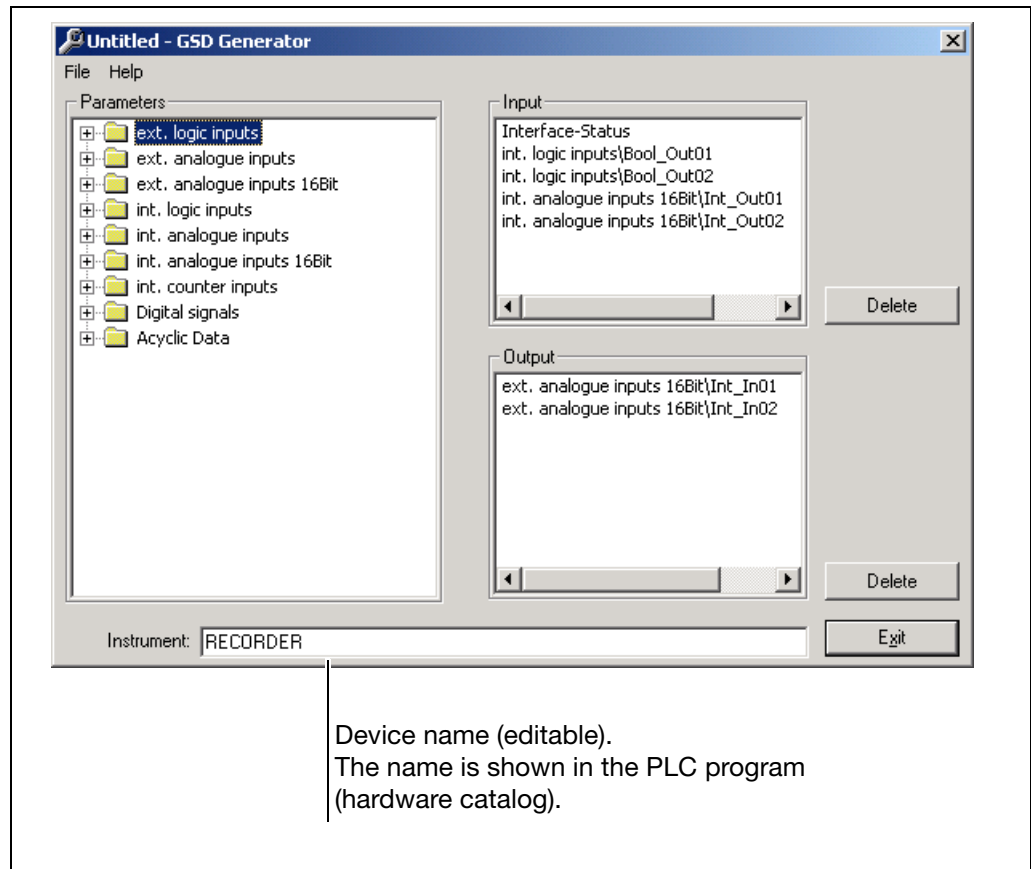

A click with the left mouse button on the “+” (⊕-📁 int. analogue inputs 16Bit) symbol or “-” (📁- int. analogue inputs 16Bit) will extend the parameter list or reduce it.

Click on the parameter with the left mouse button, and, keeping it pressed, copy it to the input or output window by Drag & Drop.

## Remove parameter

Parameters are deleted from the input or output window using the corresponding **Delete** button.



The parameter “Interface status” will automatically appear in the input window and cannot be deleted. It is used for diagnosis of the internal data transmission in the device and can be requested by the PLC:

- 0 : internal communication in device is OK
- unequal 0 : faulty communication in device

# 3 Configuring a PROFIBUS system

## 3.4 Connection example


The example below shows the path for the connection of a recorder to a S7 from Siemens.

### 3.4.1 RECORDER


- \* Connect the device to the PLC.
- \* Set the device address.  
The device (instrument) address can be selected via the instrument keys or through the setup program.

### 3.4.2 GSD generator

- \* Start up the GSD generator (Example: *Start* → *Programs* → *OEM devices* → *Profibus* → *GSD generator*).
- \* Select the recorder.

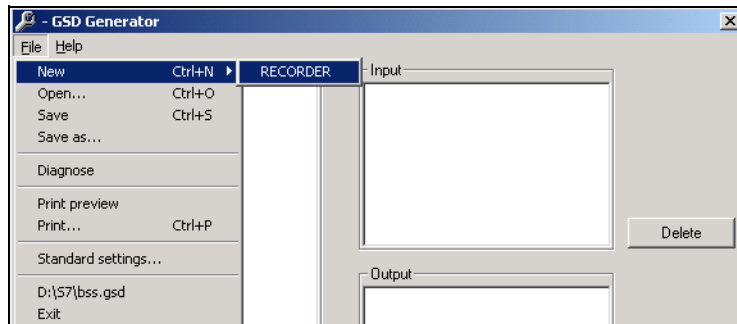


- \* Select the variables that are transmitted to the master.

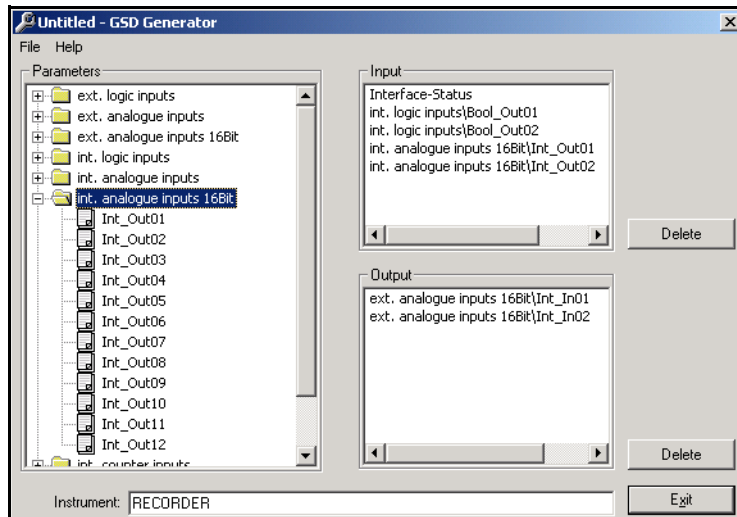


## 3 Configuring a PROFIBUS system

- \* Save the GSD file in any folder.

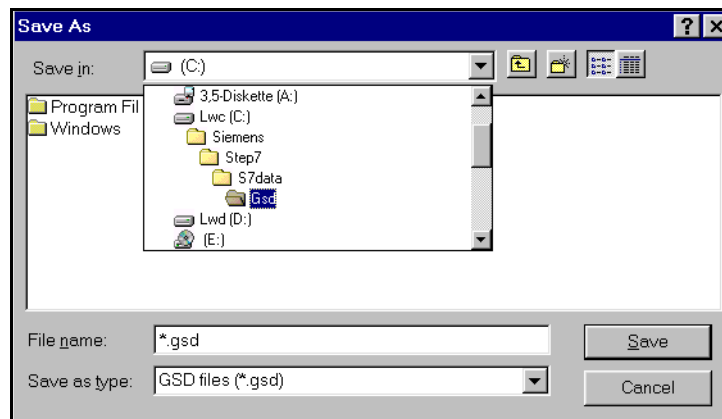

### 3.4.3 PLC configuration


- \* Start the PLC software.
- \* Call up the hardware configuration and execute menu command "Install new GSE".

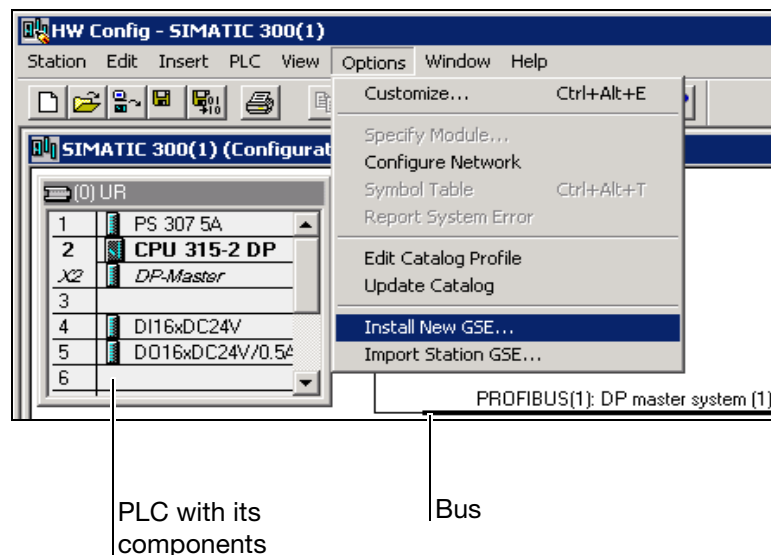

The new GSD file is read in and processed, and the recorder is inserted in the hardware catalog.


## 3 Configuring a PROFIBUS system

- \* Open the hardware catalog and place the new device in the working area.

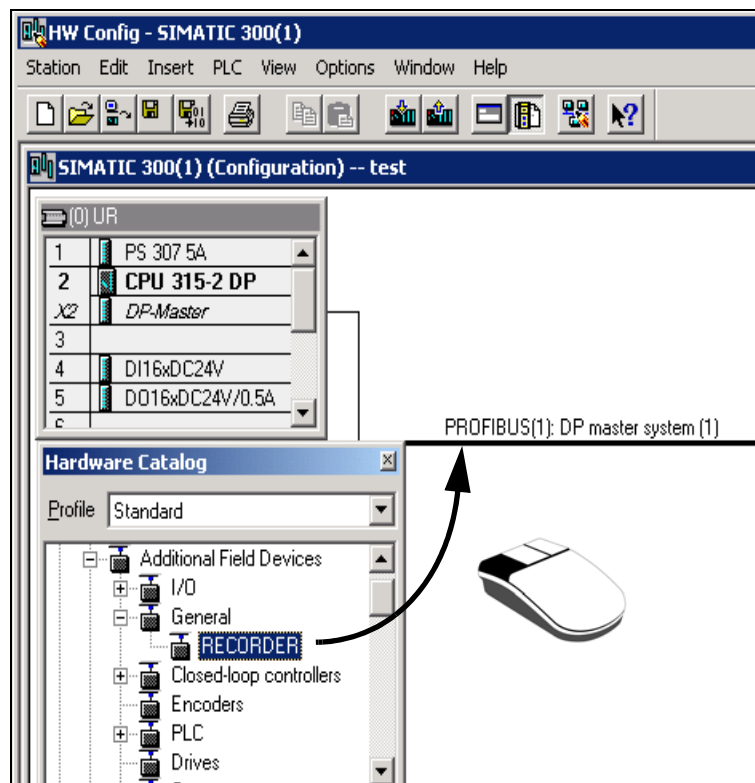

The recorder is placed on the bus using the left mouse button. After releasing the mouse button, the recorder address has to be assigned. The baud rate is determined automatically.

- \* Finally, you have to load the configuration into the PLC (*PLC* → *Download to module*)

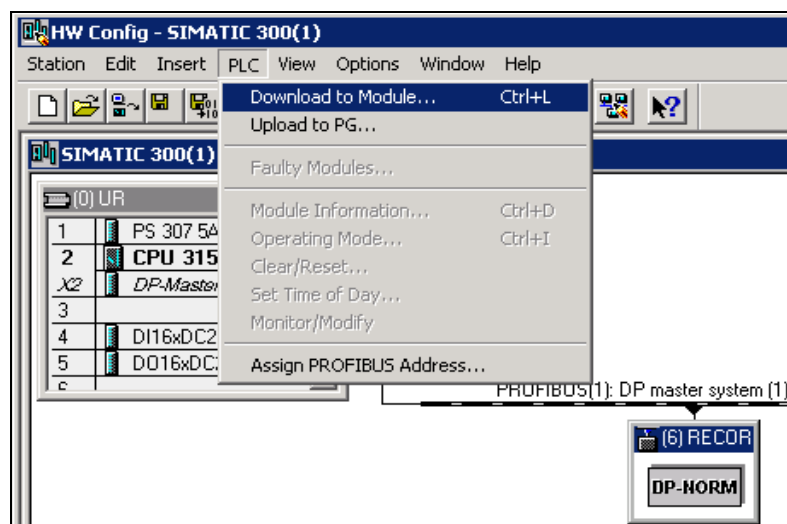

# 3 Configuring a PROFIBUS system

---

## 4 Data format of the recorder

---

When using recorders in a PROFIBUS DP system, please take note of their data format.

### Integer values

Integer values are transmitted in the following format:

- first the high byte,
- then the low byte.


### Float values/ real values

The float/real values of the cyclic data for the paperless recorder are transmitted using the IEEE-754 standard format (32 bits).

The float/real values for the acyclic data of the paperless recorder are transmitted in the MODbus format.

The IEEE-754 standard format and the MODbus format differ in the transmission sequence of the individual bytes. In the MODbus format bytes 1 and 2 are swapped with bytes 3 and 4 (first the high byte, then the low byte).

#### Single-float format (32bits) as per IEEE 754 standard



S - sign bit (bit31)

E - exponent in complement to base 2 (bit23 — bit30)

M - 23bit normalized mantissa (bit0 — bit22)

Example:

calculation of the real number from sign, exponent and mantissa.

byte1 = 40h, byte2 = F0, byte 3 = 0, byte 4 = 0

40F00000h = 0100 0000 1111 0000 0000 0000 0000 0000b

S = 0

E = 100 0000 1


M = 111 0000 0000 0000 0000 0000

$$\text{Value} = -1^S \cdot 2^{\text{exponent}-127} \cdot (1 + M_{b22} \cdot 2^{-1} + M_{b21} \cdot 2^{-2} + M_{b20} \cdot 2^{-3} + M_{b19} \cdot 2^{-4} + \dots)$$
$$\text{Value} = -1^0 \cdot 2^{129-127} \cdot (1 + 1 \cdot 2^{-1} + 1 \cdot 2^{-2} + 1 \cdot 2^{-3} + 0 \cdot 2^{-4})$$
$$\text{Value} = 1 \cdot 2^2 \cdot (1 + 0.5 + 0.25 + 0.125 + 0)$$
$$\text{Value} = 1 \cdot 4 \cdot 1.875$$
$$\text{Value} = 7.5$$

## 4 Data format of the recorder

---


### MODbus float format

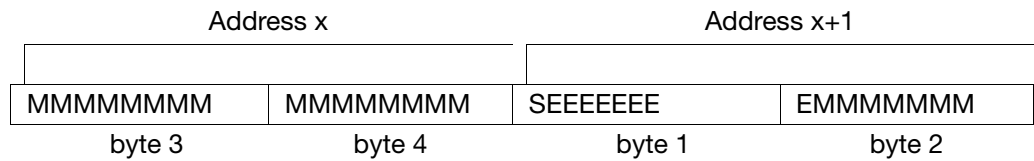

After/before the transmission from/to the device, the bytes of the float value have to be swapped accordingly.

Many compilers (e.g. Microsoft C++, Turbo C++, Turbo Pascal, Keil C51) store the float values in the following order (Intel compatibility):

### float value

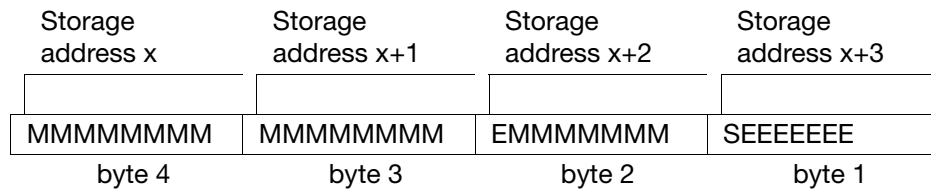

Please check how float values are stored in your application. If necessary, the bytes have to be swapped accordingly.

## 5 Device-specific data

---

This chapter describes the connection of the

- paperless recorder LOGOSCREEN, or the
  - paperless recorder LOGOSCREEN es
- to the PROFIBUS DP.



All the devices described can be used exclusively as DP slaves.

## 5 Device-specific data

### 5.1 Paperless recorder LOGOSCREEN

The paperless recorder can be used to record and display, amongst other inputs, up to 36 analog channels from a PLC.

### 5.2 System requirements


The following requirements must be met when connecting a paperless recorder to the PROFIBUS DP:

- Fit the PROFIBUS DP interface to the paperless recorder
- Program version from 100.03.02

The program version can be requested from the paperless recorder menus via *Device (Instrument) info* → *Version number*.

### 5.3 Connection diagram

Rear view of  
paperless  
recorder

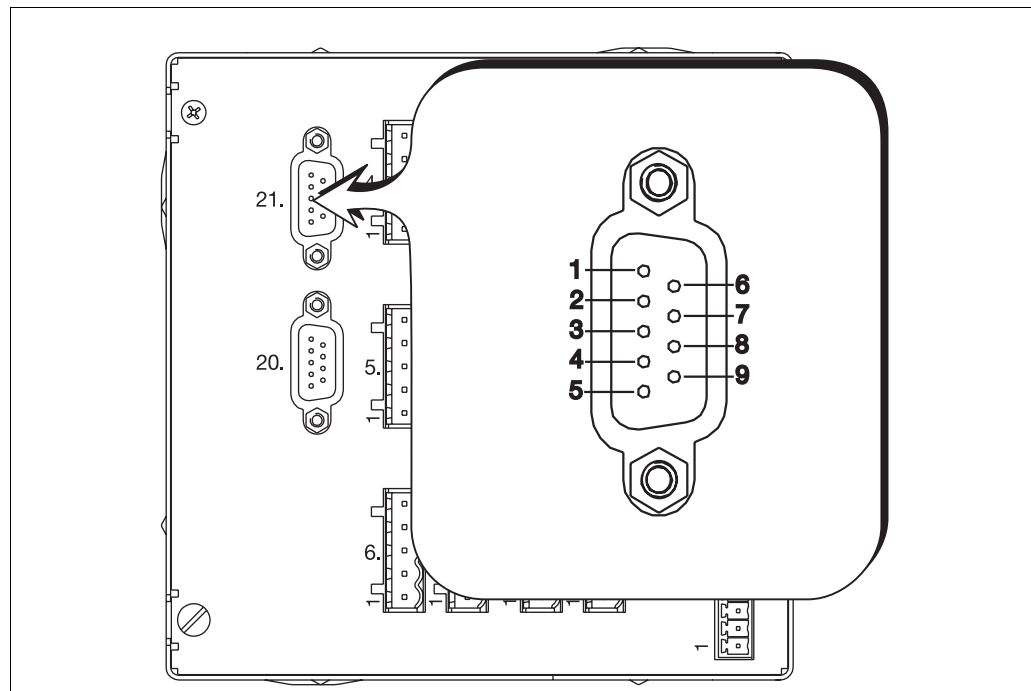

**Connector 21**

Interface

**PROFIBUS DP**

Connections

Sub-D	Signal	Designation
3	RxD/TxD-P	Receive/Transmit Data-P, B-cable
5	DGND	Data transmission ground potential
6	VP	Supply voltage-P, (P5V)
8	RxD/TxD-N	Receive/Transmit data-N, A-cable



When making the connection to the PROFIBUS DP it is important to ensure that the connectors 20 and 21 are not swapped. Connector 20 is reserved for the serial interface. The serial interface is used to read out instrument and process data from the paperless recorder. The connection and function of the serial interface are described in the Interface Description.

### 5.4 Setting the slave address

The slave address is set via the paperless recorder or the setup program.

Setting	Meaning
1 – 124	Slave address, as selected
125	The setting of the slave address can be predefined by the bus master

The baud rate is determined automatically (max. 12Mbps).

If a new device address is selected, the device has to be reset (switch off/on) for the new address to be accepted.

### 5.5 Diagnostic and status messages

If errors occur during communication with the device, a message appears in the header (**i**) and in the “Instrument info” menu.

Please check the wiring and the master (PLC). It may be necessary to restart the system.

### 5.6 Acyclic data

You can read and write different measurement and process data of the paperless recorder with “acyclic data” (from program version 100.03.03).



The acyclic data, too, can be transmitted through the cyclic data transfer.

In order to establish the communication with the paperless recorder (device), it must receive 3 info bytes and a maximum of 10 bytes of actual data.

#### Protocol structure

Byte No.	1	2	3	4 – 13
contents	control byte	function	address	actual data

## 5 Device-specific data

---

**Control byte** The control byte (byte No. 1) is organized as follows:

bit 0 – 3: length of actual data (in words)

bit 4 – 5: "toggle flag"

The two bits have their state changed (toggled) with every new job that is sent to the device so that it can recognize the new command. The bits may only be transmitted after the transmit buffer has been fully prepared for the new command.

Example:

Bit 5	Bit 4	
0	0	no job present
0	1	bit 4 is set, job 1 is being processed
1	0	bit 5 is set, job 2 is being processed
0	1	bit 4 is set, job 3 is being processed
...	...	.....

bit 6 – 7: Response OK: bit 6 = 0 and bit 7 = 1

Response faulty: bit 6 = 1 and bit 7 = 0

Bits 6 and 7 are a signal to the PLC that the command has been processed by the device and the next command to the device can be generated and transmitted by the PLC.

Bit 7	Bit 6	Bit 5	Bit 4	
0	0	0	1	bits 4 and 5 are returned unchanged by the device as a "job is being processed" info
0	0	1	0	bits 4 and 5 are returned unchanged by the device as a "job is being processed" info
1	0	0	1	fault-free processing of job with bit 4 = 1
0	1	0	1	processing of job with bit 4 = 1 was not fault-free
0	0	1	0	bits 4 and 5 are returned unchanged by the device as a "job is being processed" info
1	0	1	0	fault-free processing of job with bit 5 = 1
0	1	1	0	processing of job with bit 5 = 1 was not fault-free
...	...	...	...	.....

**Function** 03x: read  
10x: write

**Address** The addresses below can be read and written. The list corresponds to a portion of the addresses that are contained in the interface description of the paperless recorder.

The address that is defined in the protocol is calculated as follows:

**address = base address + address of variable**

Example: address for the measurement of analog input 6:

**address = 0x35 + 0x0A = 0x3F**

## 5 Device-specific data

Base address: 0x35

Address of variable	Access	Data type	Signal designation
0x00	R/O	real	Meas. input 1 (analog input 1)
0x02	R/O	real	Meas. input 2 (analog input 2)
0x04	R/O	real	Meas. input 3 (analog input 3)
0x06	R/O	real	Meas. input 4 (analog input 4)
0x08	R/O	real	Meas. input 5 (analog input 5)
0x0A	R/O	real	Meas. input 6 (analog input 6)
0x0C	R/O	real	Meas. input 7 (analog input 7)
0x0E	R/O	real	Meas. input 8 (analog input 8)
0x10	R/O	real	Meas. input 9 (analog input 9)
0x12	R/O	real	Meas. input 10 (analog input 10)
0x14	R/O	real	Meas. input 11 (analog input 11)
0x16	R/O	real	Meas. input 12 (analog input 12)
0x18	R/O	real	not used
0x1A	R/O	real	not used
0x1C	R/O	real	not used
0x1E	R/O	real	not used
0x20	R/O	real	Counter value 1
0x22	R/O	real	Counter value 2
0x24	R/O	real	External counter value 1 (from external I/O modules)
0x26	R/O	real	External counter value 2 (from external I/O modules)
0x28	R/W	real	External analog input 1 (from external I/O modules or via MODbus)
0x2A	R/W	real	External analog input 2
0x2C	R/W	real	External analog input 3
0x2E	R/W	real	External analog input 4
0x30	R/W	real	External analog input 5
0x32	R/W	real	External analog input 6
0x34	R/W	real	External analog input 7
0x36	R/W	real	External analog input 8

## 5 Device-specific data

---

0x38	R/W	real	External analog input 9
0x3A	R/W	real	External analog input 10
0x3C	R/W	real	External analog input 11
0x3E	R/W	real	External analog input 12
0x40	R/W	real	External analog input 13
0x42	R/W	real	External analog input 14
0x44	R/W	real	External analog input 15
0x46	R/W	real	External analog input 16
0x48	R/W	real	External analog input 17
0x4A	R/W	real	External analog input 18
0x4C	R/W	real	External analog input 19
0x4E	R/W	real	External analog input 20
0x50	R/W	real	External analog input 21
0x52	R/W	real	External analog input 22
0x54	R/W	real	External analog input 23
0x56	R/W	real	External analog input 24
0x58	R/W	real	External analog input 25
0x5A	R/W	real	External analog input 26
0x5C	R/W	real	External analog input 27
0x5E	R/W	real	External analog input 28
0x60	R/W	real	External analog input 29
0x62	R/W	real	External analog input 30
0x64	R/W	real	External analog input 31
0x66	R/W	real	External analog input 32
0x68	R/W	real	External analog input 33
0x6A	R/W	real	External analog input 34
0x6C	R/W	real	External analog input 35
0x6E	R/W	real	External analog input 36

## 5 Device-specific data

Base address: 0xA6

Address of variable	Access	Data type	Signal designation
0x00	R/W	char 21	Text 1 for batch report
0x0B	R/W	char 21	Text 2 for batch report
0x16	R/W	char 21	Text 3 for batch report
0x21	R/W	char 21	Text 4 for batch report



Addresses are defined as bytes in the report, addressing of data word by word.

### Actual data

A maximum of 10 bytes actual data may be defined. The number of the actual data being used (in words) is stored in bits 4 – 13.

### Command sequence

- PLC sends job 1
  - PLC sets bit 4 in the control byte
  - PLC receives the answer “job OK” or “job faulty”
- PLC sends job 2
  - PLC resets bit 4 in the control byte and sets bit 5
  - PLC receives the answer “job OK” or “job faulty”
- PLC sends job 3
  - PLC resets bit 5 in the control byte and sets bit 4
  - PLC receives the answer “job OK” or “job faulty”
- and so on.

### Example (write):

Text 1 for the batch report has to be written. Since a batch text may consist of up to 20 characters, it is transmitted in 2 parts with 10 characters each. Character 21 (0x) can be dispensed with.

The following bytes have to be transmitted to the recorder:

#### a.) Byte 1 – 10

0x25	0x10	0xA6	0x54	0x68	0x75	0x65	0x72	0x69	0x6E	0x67	0x65	0x72
						A	c	e	t	y	l	-

#### b.) Byte 11 – 20

0x15	0x10	0xAB	0x2D	0x42	0x72	0x61	0x74	0x77	0x75	0x72	0x73	0x74
									a	c	i	d



When sending the first 10 characters, the start address is 0xA6. Since addressing is done word by word, the second 10 characters have to be sent with the address from 0xAB (0xA6 + 5).

# 5 Device-specific data

## 5.7 PLC data in 16-bit format

The functions described below can only be implemented on paperless recorders from program version 100.03.05.

### Internal measurement inputs of the paperless recorder

From program version 100.03.05, the internal measurement inputs (1 – 6 or 1 – 12) can not only be sent to the PROFIBUS master (PLC) in “Real” format (4 bytes), but also in “Integer” format (2 bytes).


Using the setup program for the paperless recorder, four values for measurement standardization have to be entered for **all internal channels** (not for each individually).

- range start
- range end
- value at underrange
- value at overrange

The internal measurements are converted from “Real” format to “Integer” format. In order to enable a uniform conversion, these four parameters have been inserted.

The parameters are entered in the field “Interface 21”.

The dialog can be called up by a double click on the working area, or through the menu *Edit* → *Interface 21 (PROFIBUS DP)*.

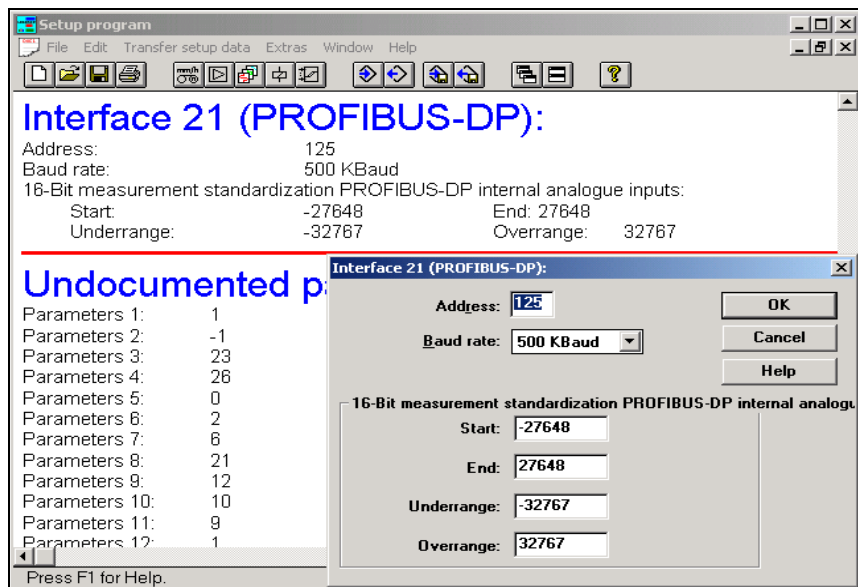

### External measurement inputs of the paperless recorder

The external measurement inputs (1 – 36) can also be sent to the paperless recorder, either in “Real” format (4 bytes), or “Integer” format (2 bytes). Which data format is to be used, can also be decided with the help of the GSD generator.


With the “Integer” format, the parameters *Range start* and *Range end* are used to carry out standardization to 16 bits. This can be done through the setup program, or from the instrument keys.

# 5 Device-specific data

The analog input of the PLC provides a 16-bit measurement in the range from -27648 to +27648; the ranges depend on the input sensor that was selected or the input card being used.

## Example


	Input meas. range of PLC	Standardization range of PLC	Range paperless recorder	Scaling paperless recorder
Range start	-10V	-27648	-27648	-10
Range end	+10V	+27648	+27648	+10

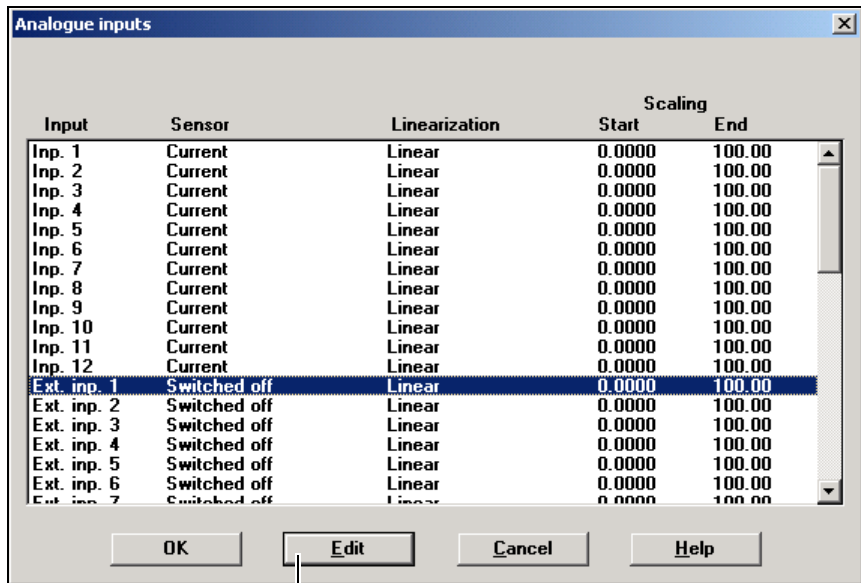

First of all, the "Edit" button has to be activated for the external measurement inputs, ...

... then the external input can be activated and ...

... finally, standardization can be carried out.

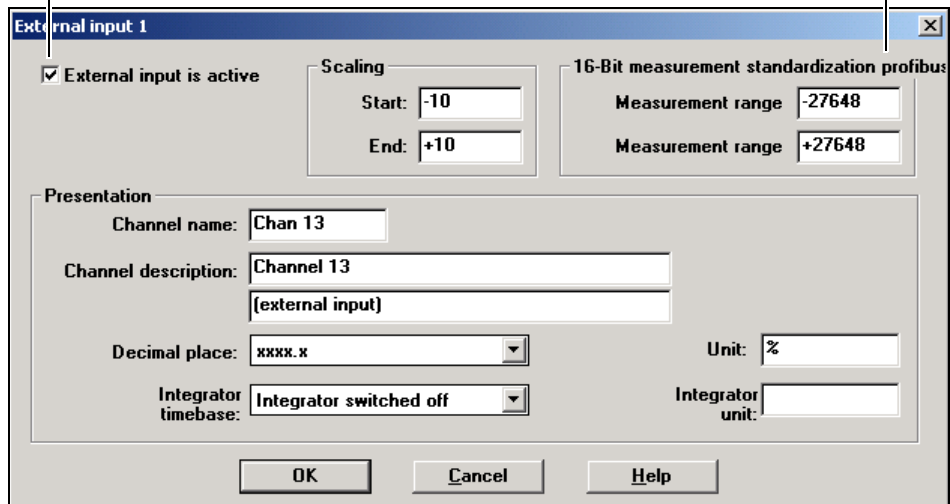

## 5 Device-specific data

---

### 5.8 Bit-by-bit coding of binary signals

The signals described below are available for paperless recorders with program version 100.03.05 or above and can be addressed using the GSD generator.

Address	Access	Data type	Signal designation
Alarm_Group1-6	R/O	bit0	Alarm group 1 0 = no alarm 1 = at least 1 limit infringed in group
	R/O	bit1	Alarm group 2
	R/O	bit2	Alarm group 3
	R/O	bit3	Alarm group 4
	R/O	bit4	Alarm group 5
	R/O	bit5	Alarm group 6
	R/O	bit6-7	not used
Int. logic inp. 1-7	R/O	bit0	Logic input 1 0 = open / 1 = closed
	R/O	bit1	Logic input 2
	R/O	bit2	Logic input 3
	R/O	bit3	Logic input 4
	R/O	bit4	Logic input 5
	R/O	bit5	Logic input 6
	R/O	bit6	Logic input 7
	R/O	bit7	not used
Additional_ dig.signals	R/O	bit0	Combination alarm 0 = no alarm 1 = at least 1 limit infringed in device
	R/O	bit1	Diskette reserve signal 0 = disk. reserve not yet reached 1 = replace diskette
	R/O	bit2	Fault 0 = no fault / 1 = fault
	R/O	bit3-7	not used

## 5 Device-specific data

---

Address	Access	Data type	Signal designation
Output1-6	R/O	bit0	Relay output 1 0 = not active / 1 = active
	R/O	bit1	Relay output 2
	R/O	bit2	Relay output 3
	R/O	bit3	Relay output 4
	R/O	bit4	Relay output 5
	R/O	bit5	Open-collector output 0 = not active / 1 = active
	R/O	bit6-7	not used
Ext.logic inp.1-6	R/W	bit0	External logic input 1 0 = open / 1 = closed
	R/W	bit1	External logic input 2
	R/W	bit2	External logic input 3
	R/W	bit3	External logic input 4
	R/W	bit4	External logic input 5
	R/W	bit5	External logic input 6
	R/W	bit6-7	not used

### 5.9 External inputs and faults in the data exchange

As long as there is no data exchange between the PLC and the recorder, the external analog inputs of the recorder are treated as “invalid” (display -----). Thus it is possible to detect, during the evaluation of the measurement data, that there were no valid values present for this period. This only applies to the external measurement inputs.

All other data (binary signals, batch texts, ...) will be frozen and remain at their current values.

## 5 Device-specific data

### 5.10 Paperless recorders LOGOSCREEN es and cf

A paperless recorder can be used to record and display, amongst other inputs, up to 36 analog channels from a PLC.

#### 5.10.1 System requirements

The following conditions must be fulfilled in order to connect a paperless recorder to the PROFIBUS DP interface:


- Paperless recorder with a PROFIBUS DP interface



If a plug-in card for PROFIBUS DP is fitted, then *PROFIBUS DP* appears as an entry in the *Device Info* menu for *Interface 2*.

#### 5.10.2 Connections for LOGOSCREEN es and cf

Rear view of the paperless recorder

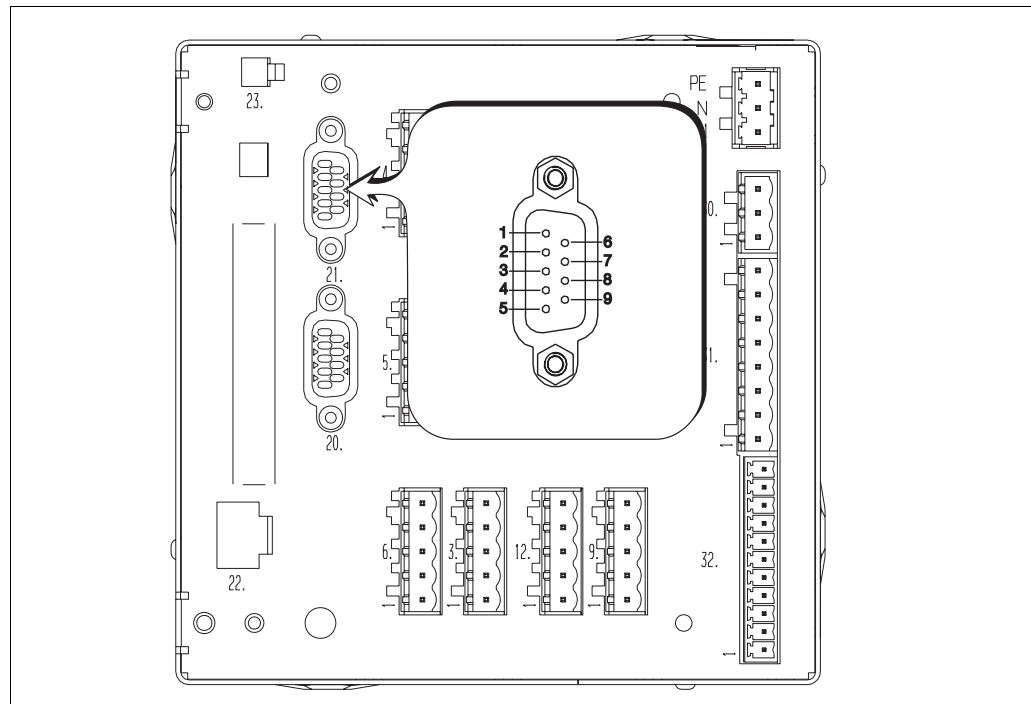

**Connector 21**

Interface

**PROFIBUS DP**

Connections

Sub-D	Signal	Designation
3	RxD/TxD-P	Receive/Transmit Data-P, B-cable
5	DGND	Data transmission ground potential
6	VP	Supply voltage-P, (P5V)
8	RxD/TxD-N	Receive/Transmit data-N, A-cable



When making the connection to the PROFIBUS DP it is important to ensure that the connectors 20 and 21 are not swapped. Connector 20 is reserved for the serial interface. The serial interface is used to read out device and process data from the paperless recorder. The connection and function of the serial interface are described in the Interface Description B 70.6560.2.0.

### 5.10.3 Setting the slave address

The slave address is set with the help of the paperless recorder or the setup program.

Setting	Meaning
1 – 124	Slave address, as set
125	The setting for the slave address can be predefined by the bus master.

The baud rate is determined automatically (max. 12Mbps).

### 5.10.4 Diagnosis and status messages

If errors occur during communication with the device, the **(i)** symbol in the header line will blink, and an error message appears in the *Device info* menu. The measurements are labeled as *invalid* (200003). The screen of the Logoscreen displays "-----". Please check the wiring and the master (PLC). It may be necessary to restart the system.

#### Suppression

The error messages in the *Device info* menu and the **(i)** in the header can be suppressed by setting the slave address to 125.

### 5.10.5 Acyclic data transmission

You can use the *acyclic data* function to read and write various measurement and process data of the paperless recorder



Acyclic data can also be transmitted by means of cyclic data transfer.

In order to establish communication with the paperless recorder (the device), it must receive 3 info bytes and a maximum of 10 bytes of actual data.

#### Protocol structure

Byte No.	1	2	3	4 ... 13
contents	control byte	function	address	actual data

## 5 Device-specific data

---

**Control byte** The control byte (byte No. 1) is organized as follows:

bit 0 – 3: length of actual data (in words)

bit 4 – 5: "toggle flag"

Boths bits must change state (toggle) with every new job that is sent to the device, so that it can recognize the new command. The bits must only be set after the transmit buffer has been fully prepared for the new command.

Example:

Bit 5	Bit 4	
0	0	no job present
0	1	bit 4 is set, job 1 is being processed
1	0	bit 5 is set, job 2 is being processed
0	1	bit 4 is set, job 3 is being processed
...	...	.....

bit 6 – 7: Response OK: bit 6 = 0 and bit 7 = 1

Response faulty: bit 6 = 1 and bit 7 = 0

Bit 6 and bit 7 are a signal for the PLC that the command has been processed by the device, and the next command for the device can be generated and transmitted by the PLC.

Bit 7	Bit 6	Bit 5	Bit 4	
0	0	0	1	bits 4 and 5 are returned unchanged by the device as a "job is being processed" info
0	0	1	0	bits 4 and 5 are returned unchanged by the device as a "job is being processed" info
1	0	0	1	fault-free processing of job with bit 4 = 1
0	1	0	1	processing of job with bit 4 = 1 was not fault-free
0	0	1	0	bits 4 and 5 are returned unchanged by the device as a "job is being processed" info
1	0	1	0	fault-free processing of job with bit 5 = 1
0	1	1	0	processing of job with bit 5 = 1 was not fault-free
...	...	...	...	.....

**Function** 0x03: read  
0x10: write

### 5.10.6 Extension of the address range for LOGOSCREEN es and cf

The (previously) unused bits 7, 6 and 5 from the function byte are used to form an 11-bit wide Modbus address.

## 5 Device-specific data

Function byte	Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0			
	1	1	1	0000 1010 read or 0000 0011 write							
Address byte	Bit10	Bit9	Bit8	Bit 7	Bit 6	Bit 5	Bit 4	Bit 3	Bit 2	Bit 1	Bit 0
	1	1	1	1	1	1	1	1	1	1	1
Highest address	7			F				F			

### Address

The following addresses can be read and written. The list corresponds to a portion of the addresses which are contained in the interface description of the paperless recorder.

The address that is defined in the protocol is derived from:

$$\text{address} = \text{base address} + \text{address of variable}$$

Example: the address for the measurement of analog input 6 is:

$$\text{address} = 0x35 + 0x0A = 0x3F$$

### 5.10.7 Process data

Base address: 0x002F

Address	Access	Data type	Signal designation
0x0000	R/O	int	Group alarm and logic input settings
	R/O	bit0	Alarm group 1 0 = no alarm 1 = at least 1 limit infringement in the group
	R/O	bit1	Alarm group 2
	R/O	bit2	Alarm group 3
	R/O	bit3	Alarm group 4
	R/O	bit4	Alarm group 5
	R/O	bit5	Alarm group 6
	R/O	bit6-7	not used
	R/O	bit8	Logic input 1 0 = open / 1 = closed
	R/O	bit9	Logic input 2
	R/O	bit10	Logic input 3

## 5 Device-specific data

---

Address	Access	Data type	Signal designation
	R/O	bit11	Logic input 4
	R/O	bit12	Logic input 5
	R/O	bit13	Logic input 6
	R/O	bit14	Logic input 7
	R/O	bit15	not used
0x0001	R/O	int	Logic signals
	R/O	bit0	CompactFlash card is in the slot (0 = no, 1 = yes)
	R/O	bit1	CF card has been stolen (0 = no, 1 = card was removed while no user was logged in)
	R/O	bit2	Memory alarm: insufficient free internal memory available. Data must be fetched on a CF card!
	R/O	bit3	Memory alarm: insufficient free internal memory available. Data must be fetched via the serial interface!
	R/O	bit4	Memory alarm: insufficient free memory available on the CompactFlash card!
	R/O	bit5	Login status: 0 = no user logged in 1 = a user is logged in
	R/O	bit6	not used
	R/O	bit7	not used
	R/O	bit8	Combination alarm 0 = no alarm 1 = at least 1 limit infringed in the device
	R/O	bit9	not used
	R/O	bit10	Fault condition 0 = no fault / 1 = fault
	R/O	bit11-15	not used
0x0002	R/O	int	Logic outputs
	R/O	bit0	Relay output 1 0 = not active / 1 = active
	R/O	bit1	Relay output 2
	R/O	bit2	Relay output 3

## 5 Device-specific data

Address	Access	Data type	Signal designation
	R/O	bit3	Relay output 4
	R/O	bit4	Relay output 5
	R/O	bit5	Open-collector output 0 = not active / 1 = active
	R/O	bit6-15	not used
0x0003	R/W	int	External logic inputs (either from external I/O modules or via Modbus)
	R/W	bit0	External logic input 1 0 = open / 1 = closed
	R/W	bit1	External logic input 2
	R/W	bit2	External logic input 3
	R/W	bit3	External logic input 4
	R/W	bit4	External logic input 5
	R/W	bit5	External logic input 6
	R/W	bit6-15	not used
0x0004	R/W	int	Flag for operating various device functions
	R/W	bit0	Modbus flag (control flag) 0 = false / 1 = true
	R/W	bit1-15	not used

Base address: 0x0035

Address	Access	Data type	Signal designation
0x0000	R/O	float	Measurement input 1 (analog input 1)
0x0002	R/O	float	Measurement input 2 (analog input 2)
0x0004	R/O	float	Measurement input 3 (analog input 3)
0x0006	R/O	float	Measurement input 4 (analog input 4)
0x0008	R/O	float	Measurement input 5 (analog input 5)
0x000A	R/O	float	Measurement input 6 (analog input 6)
0x000C	R/O	float	Measurement input 7 (analog input 7)
0x000E	R/O	float	Measurement input 8 (analog input 8)
0x0010	R/O	float	Measurement input 9 (analog input 9)
0x0012	R/O	float	Meas. input 10 (analog input 10)

## 5 Device-specific data

---

0x0014	R/O	float	Meas. input 11 (analog input 11)
0x0016	R/O	float	Meas. input 12 (analog input 12)
0x0018	R/O	float	not used
0x001A	R/O	float	not used
0x001C	R/O	float	not used
0x001E	R/O	float	not used
0x0020	R/O	float	Counter value 1
0x0022	R/O	float	Counter value 2
0x0024	R/O	float	External counter value 1 (from external I/O modules)
0x0026	R/O	float	External counter value 2 (from external I/O modules)
0x0028	R/W	float	External analog input 1 (from external I/O modules or via Modbus)
0x002A	R/W	float	External analog input 2
0x002C	R/W	float	External analog input 3
0x002E	R/W	float	External analog input 4
0x0030	R/W	float	External analog input 5
0x0032	R/W	float	External analog input 6
0x0034	R/W	float	External analog input 7
0x0036	R/W	float	External analog input 8
0x0038	R/W	float	External analog input 9
0x003A	R/W	float	External analog input 10
0x003C	R/W	float	External analog input 11
0x003E	R/W	float	External analog input 12
0x0040	R/W	float	External analog input 13
0x0042	R/W	float	External analog input 14
0x0044	R/W	float	External analog input 15
0x0046	R/W	float	External analog input 16
0x0048	R/W	float	External analog input 17
0x004A	R/W	float	External analog input 18
0x004C	R/W	float	External analog input 19

## 5 Device-specific data

0x004E	R/W	float	External analog input 20
0x0050	R/W	float	External analog input 21
0x0052	R/W	float	External analog input 22
0x0054	R/W	float	External analog input 23
0x0056	R/W	float	External analog input 24
0x0058	R/W	float	External analog input 25
0x005A	R/W	float	External analog input 26
0x005C	R/W	float	External analog input 27
0x005E	R/W	float	External analog input 28
0x0060	R/W	float	External analog input 29
0x0062	R/W	float	External analog input 30
0x0064	R/W	float	External analog input 31
0x0066	R/W	float	External analog input 32
0x0068	R/W	float	External analog input 33
0x006A	R/W	float	External analog input 34
0x006C	R/W	float	External analog input 35
0x006E	R/W	float	External analog input 36

Base address: 0x00A6

Address	Access	Data type	Signal designation
0x0000	R/W	char 21	Text 1 for batch reports
0x000B	R/W	char 21	Text 2 for batch reports
0x0016	R/W	char 21	Text 3 for batch reports
0x0021	R/W	char 21	Text 4 for batch reports
0x002C	R/W	char 21	Text 5 for batch reports
0x0037	R/W	char 21	Text 6 for batch reports
0x0042	R/W	char 21	Text 7 for batch reports
0x004D	R/W	char 21	Text 8 for batch reports
0x0058	R/W	char 21	Text 9 for batch reports
0x0063	R/W	char 21	Text 10 for batch reports

## 5 Device-specific data

---

Base address: 0x0114

Address	Access	Data type	Signal designation
0x0000	R/W	char 21	Message text (for the entry in the event list)

Base address: 0x011F

Address	Access	Data type	Signal designation
0x0000	W/O	char 11	Only for LOGOSCREEN cf: Password
0x0006	R/O	12 Byte	(*) reserved

Base address: 0x012B

Address	Access	Data type	Signal designation
0x0000	R/W	char 400	Recipe for batch reports



External logic inputs (R/W), external counters (R/O) and external analog inputs (R/W) can be programmed via the serial interface or connected to the paperless recorder in the form of modules of the JUMO mTRON automation system. For additional information, please refer to the Operating Instructions 70.6560.2.1 (LON interface).



The address is given byte-wise in the protocol.  
The data are addressed word-wise.

### User data

A maximum of 10 bytes of user data can be presented. The quantity of user data is given (in words) by bits 4 – 13.

### Command sequence

- PLC sends 1st job
  - PLC sets bit 4 in the control byte
  - PLC receives response “job OK” or “job faulty”
- PLC sends 2nd job
  - PLC resets bit 4 in the control byte and sets bit 5
  - PLC receives response “job OK” or “job faulty”
- PLC sends 3rd job
  - PLC resets bit 5 in the control byte and sets bit 4
  - PLC receives response “job OK” or “job faulty”
- and so on ...

## 5 Device-specific data

---

**Example  
(write):**

Text 1 for the batch report has to be written- Since a batch text can have a maximum of 20 characters, it will be transmitted in 2 sections, each consisting of 10 characters. The 21st character (0x) can be left out.

The following bytes must be transmitted to the recorder:

**a.) Bytes 1 – 10**

0x25	0x10	0xA6	0x54	0x68	0x75	0x65	0x72	0x69	0x6E	0x67	0x65	0x72
						A	c	e	t	y	l	-

**b.) Bytes 11 – 20**

0x15	0x10	0xAB	0x2D	0x42	0x72	0x61	0x74	0x77	0x75	0x72	0x73	0x74
									a	c	i	d



The starting address for transmitting the first 10 characters is 0xA6. Since addressing is carried out word-wise, the second 10 characters must be addressed from 0xAB (0xA6 + 5) onwards for transmission.

# 5 Device-specific data

## 5.10.8 PLC data in 16-bit format

The functions described below are only available for paperless recorders with a program version 100.03.05 or above.

### Internal measurement inputs to the paperless recorder

From program version 100.03.05 on, the internal measurement inputs (1 – 6 or 1 – 12) can be transmitted to the PROFIBUS master (the PLC) not only in *real* format ( 4 bytes) but also in *integer* format (2 bytes).


It is necessary to use the setup program of the recorder to enter four values for the normalization of the measurements **for all the internal channels** (i.e. not separately for each channel):

- Measurement range start
- Measurement range end
- Value for underrange
- Value for overrange

The internal measurement values are converted from the real format into the integer format. These four parameters have been introduced in order to enable a uniform conversion calculation for all channels.

The parameters are entered in the section *Interface 21*.

Call up the dialog by a double-click inside the working area, or through the menu *Edit* → *Interface 21 (PROFIBUS DP)*

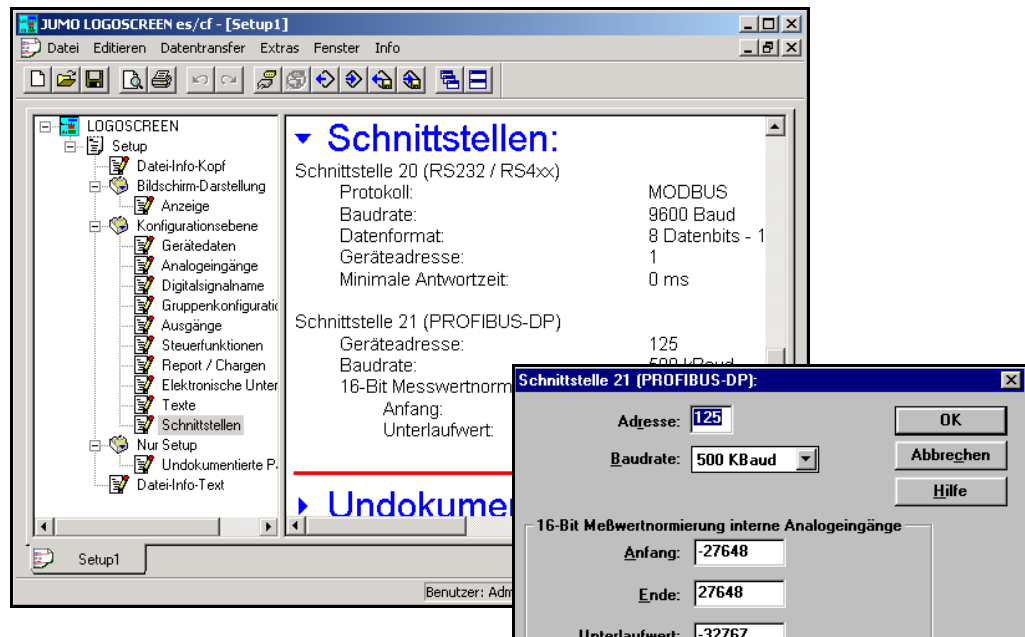

### External measurement inputs to the paperless recorder

The external measurement inputs (1 – 36) can also be transmitted to the recorder in real format (4 bytes) as well as in integer format (2 bytes). The decision as to which data form should be used is also made with the aid of the GSD generator.

When using the *integer* format, the parameters *Measurement range start* and *Measurement range end* must be set for 16-bit normalization. This can be done either through the setup program, or using the keypad on the recorder.

## 5 Device-specific data

The analog input of the PLC provides a 16-bit measurement signal within the range from -27648 to +27648, whereby the measurement ranges depend on the type of input sensor that is selected and the input card that is used.

### Example:

	Input range of the PLC	Normalization range of the PLC	Range of the paperless recorder	Scaling of the recorder
Range start	-10V	-27648	-27648	-10
Range end	+10V	+27648	+27648	+10

For the external measurement inputs, first press the *Edit* button ...

... then you can activate the external input, and ...

... finally, set up the normalization.

## 5 Device-specific data

---

### 5.10.9 Bit-wise coded binary logic signals

The signals described below are available for paperless recorders that have a program version 100.03.05 or above, and can be accessed through the GSD generator.

Address	Access	Data type	Signal designation
Alarm_Group1-6	R/O	bit0	Alarm group 1 0 = no alarm 1 = at least 1 limit infringement within the group
	R/O	bit1	Alarm group 2
	R/O	bit2	Alarm group 3
	R/O	bit3	Alarm group 4
	R/O	bit4	Alarm group 5
	R/O	bit5	Alarm group 6
	R/O	bit6-7	not used
Int. logic inp. 1-7	R/O	bit0	Logic input 1 0 = open / 1 = closed
	R/O	bit1	Logic input 2
	R/O	bit2	Logic input 3
	R/O	bit3	Logic input 4
	R/O	bit4	Logic input 5
	R/O	bit5	Logic input 6
	R/O	bit6	Logic input 7
	R/O	bit7	not used
Additional_dig.signals	R/O	bit0	Combination alarm 0 = no alarm 1 = at least 1 limit infringed in device
	R/O	bit1	Diskette reserve signal 0 = disk. reserve not yet reached 1 = replace diskette
	R/O	bit2	Fault 0 = no fault / 1 = fault
	R/O	bit3-7	not used

## 5 Device-specific data

Address	Access	Data type	Signal designation
Output1-6	R/O	bit0	Relay output 1 0 = not active / 1 = active
	R/O	bit1	Relay output 2
	R/O	bit2	Relay output 3
	R/O	bit3	Relay output 4
	R/O	bit4	Relay output 5
	R/O	bit5	Open-collector output 0 = not active / 1 = active
	R/O	bit6-7	not used
Ext.logic inp.1-6	R/W	bit0	External logic input 1 0 = open / 1 = closed
	R/W	bit1	External logic input 2
	R/W	bit2	External logic input 3
	R/W	bit3	External logic input 4
	R/W	bit4	External logic input 5
	R/W	bit5	External logic input 6
	R/W	bit6-7	not used

### 5.10.10 External inputs and faults in the data exchange

As long as there is no data exchange between the PLC and the recorder, the external analog inputs of the recorder are treated as "invalid" (display -----). Thus it is possible to detect, during the evaluation of the measurement data, that there were no valid values present for this period. This only applies to the external measurement inputs.

All other data (binary signals, batch texts, ...) will be frozen and remain at their current values.

# 5 Device-specific data

---













**JUMO GmbH & Co. KG**

Street address:  
Moltkestraße 13 - 31  
36039 Fulda, Germany  
Delivery address:  
Mackenrodtstraße 14  
36039 Fulda, Germany  
Postal address:  
36035 Fulda, Germany  
Phone: +49 661 6003-0  
Fax: +49 661 6003-607  
e-mail: [mail@jumo.net](mailto:mail@jumo.net)  
Internet: [www.jumo.net](http://www.jumo.net)

**JUMO Instrument Co. Ltd.**

JUMO House  
Temple Bank, Riverway  
Harlow, Essex CM20 2TT, UK  
Phone: +44 1279 635533  
Fax: +44 1279 635262  
e-mail: [sales@jumo.co.uk](mailto:sales@jumo.co.uk)  
Internet: [www.jumo.co.uk](http://www.jumo.co.uk)

**JUMO Process Control, Inc.**

8 Technology Boulevard  
Canastota, NY 13032, USA  
Phone: 315-697-JUMO  
1-800-554-JUMO  
Fax: 315-697-5867  
e-mail: [info@jumo.us](mailto:info@jumo.us)  
Internet: [www.jumo.us](http://www.jumo.us)